



Contents

	page
Features	2
To operate	2
Cleaning and maintenance	3
Battery replacement	3
Troubleshooting guide	4
Technical specifications	4
Conductivity and understanding the measuring scales	5
Bluelab measurement conversion chart	6
Product guarantee	8
Cleaning kits	9
Contact details	9



Features

Fully waterproof	Battery operated
Auto on/off function	No buttons, switches or knobs
No calibration required	Daylight readable blue LED's
Provided with EC, CF, ppm 500 and ppm 700 scales	

1.0 To operate

Using the Bluelab Commercial Truncheon® Nutrient Meter (see Figure 1) to measure nutrient conductivity involves placing the probe sensor head in the solution, followed by measuring and reading conductivity values on the stem scale indicator light.

Figure 1. Bluelab Commercial Truncheon® Nutrient Meter




1 Measure conductivity

Place probe into nutrient solution and take reading as indicated by the flashing lights.

Note: If the lights are dancing between two values, the reading is between those two values. Some example readings are shown in the table below:

Lights flashing between these EC values	Repeating pattern of flashing lights (EC)	Reading EC value
0.8 and 1.0	0.8 - 1.0, 0.8 - 1.0, 0.8 - 1.0	0.9
2.8 and 3.2	2.8 - 2.8 - 3.2, 2.8 - 2.8 - 3.2	2.9
	2.8 - 3.2 - 3.2, 2.8 - 3.2 - 3.2	3.1

Note: For very cold or very hot temperatures it will take 1-2 minutes for the probe to reach solution temperature. To help decrease time taken to reach the solution temperature, place the probe in an area where there is a strong movement of solution, or stir solution with the probe.

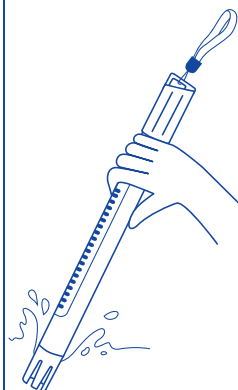

2 Obtain another reading

To take another reading, simply place back in solution.

3 Clean probe

We recommend the probe be cleaned once every two weeks according to the Cleaning and Maintenance instructions. This can vary depending on frequency of use.





2.0 Cleaning and maintenance


Cleaning the Commercial Truncheon Meter probe frequently ensures accurate readings. Clean the probe with a liquid scourer cream used in home bathrooms and kitchens such as 'Jif', 'Liquid Vim', 'Soft Scrub', 'Cif', or 'Viss'. Never use scented varieties of cleaner as they affect the probe functions.

1 Remove shroud
Twist the shroud 90 degrees and then remove the shroud.

2 Clean probe face
Place one or two drops of unscented liquid scourer, such as 'Jif', 'Liquid Vim', 'Soft Scrub', 'Cif, or 'Viss' on the probe face. Rub probe face with your finger or Bluelab Chamois firmly and vigorously to clean.

3 Rinse probe
Rinse off all traces of cleaner under running water using the same finger or other side of Bluelab Chamois. Check that the water forms a film on the probe face with no 'beads' of water. If beading is present repeat the cleaning process.

4 Replace shroud

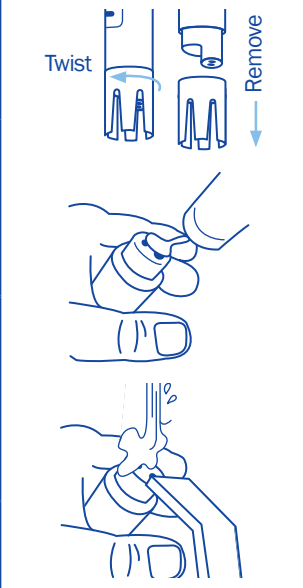

3.0 Battery replacement


The Commercial Truncheon Meter is powered with 3 x AA type standard or alkaline batteries. Do not use rechargeable batteries. Do not mix brands of batteries. Do not mix old with new. Do not put upside down. Follow these steps to replace the batteries.

1 Remove old batteries
Unfasten battery cap and tip out old batteries.

2 Check for corrosion
Batteries that have been inside the unit for a long length of time may corrode. Check battery contacts and batteries for any sign of corrosion. Contacts should be cleaned first if corrosion is found before proceeding to step 3.

3 Fit new batteries
Insert the new batteries positive (+) end down into the body.

4 Replace battery cap
Refasten battery cap. There must be no space left between the cap and body to ensure the unit remains 100% waterproof.

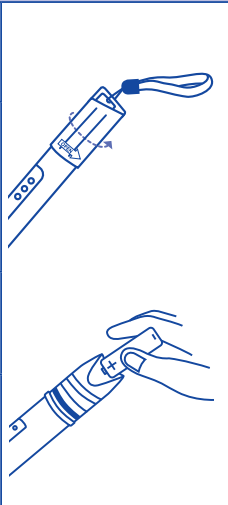



4.0 Troubleshooting guide

Trouble	Correction
<i>Truncheon Meter turns off before reading taken.</i>	Take out of solution for 3-5 seconds. Dip in solution again and take reading.
<i>Truncheon Meter not lighting when dipped in solution.</i>	Clean the probe. If this is unsuccessful, replace batteries. Do not use rechargeable batteries.
<i>Truncheon Meter gives low readings.</i>	Clean the probe. Ensure unscented cleaner is used eg. plain 'Jif', 'Soft Scrub', 'Liquid Vim', 'Cif' or 'Viss'.

5.0 Technical specifications

Range	0.4 – 6.0 EC 4 – 60 CF	200 – 3000 ppm (EC x 500) 280 – 4200 ppm (EC x 700)
Resolution	0.1 EC, 1 CF, 50 ppm (500), 70 ppm (700)	
Accuracy at 2.77EC and 25 °C / 77 °F	± 0.1 EC, ± 1 CF, ± 50 ppm (1385 ppm at 500 ppm), ± 70 ppm (1939 ppm at 700 ppm)	
Temperature compensation	Automatic	
Operating temperature	0 - 50 °C, 32 - 122 °F	
Calibration	Not required	

Limitation of liability

Under no circumstances shall BlueLab Corporation Limited be liable for any claims, losses, costs and damages of any nature whatsoever (including any consequential loss) that result from the use of, or the inability to use, these instructions.



Conductivity and understanding the measuring scales

Conductivity tells you how much food is in your solution.

Getting a grip on the different measuring scales

All these scales measure the concentration of dissolved solids in a solution. They just use different processes and scales to do so.

EC is the only absolute measure of conductivity for nutrient solutions. EC is measured in millisiemens mS/cm^2 . It's the standard everywhere outside North America. It also gives the most accurate conductivity measure. This is because different tester manufacturers use different standards to convert from EC to ppm - often resulting in inaccurate and confusing ppm readings (use our conversion chart on page 6).

CF is closely related to EC. It just doesn't have the decimal point.

ppm verses TDS. The ppm 500 scale is the same as TDS. TDS - Total Dissolved Solids - is represented as ppm by some meters. A TDS reading of 50 means that there are 50 milligrams of dissolved solids in each litre of water. 50ppm.

The ppm 700 scale as no relation to TDS, so 70 milligrams of dissolved solids in a litre of water is 70 ppm. However, the actual ppm of a solution can only be measured accurately by chemical analysis.

Understanding these scales

We saw that EC measures are the most accurate. Most ppm meters measure in EC. They then convert this to a ppm value.

The conversion factor from EC to ppm can vary, but those most widely used for measuring nutrient solutions are the 'EC x 500' scale. It is worth remembering the ppm 500 scale is sometimes called TDS.

No ifs or buts!

Measure conductivity every day.

- If you don't know which ppm scale to use, ask your nutrient manufacturer or use EC
- Avoid over-diluting or over-concentrating your nutrient solution
- Start with a quality nutrient
- Completely change the reservoir solution every 7 days
- Top up the nutrient level between changes - so your plants have the right amount of food.



Bluelab measurement conversion chart

mS/cm ² Millisiemen per cm ²	EC	CF	ppm 500 TDS	ppm 700
0.1	0.1	1	50	70
0.2	0.2	2	100	140
0.3	0.3	3	150	210
0.4	0.4	4	200	280
0.5	0.5	5	250	350
0.6	0.6	6	300	420
0.7	0.7	7	350	490
0.8	0.8	8	400	560
0.9	0.9	9	450	630
1.0	1.0	10	500	700
1.1	1.1	11	550	770
1.2	1.2	12	600	840
1.3	1.3	13	650	910
1.4	1.4	14	700	980
1.5	1.5	15	750	1050
1.6	1.6	16	800	1120
1.7	1.7	17	850	1190
1.8	1.8	18	900	1260
1.9	1.9	19	950	1330
2.0	2.0	20	1000	1400
2.1	2.1	21	1050	1470
2.2	2.2	22	1100	1540
2.3	2.3	23	1150	1610
2.4	2.4	24	1200	1680
2.5	2.5	25	1250	1750
2.6	2.6	26	1300	1820
2.7	2.7	27	1350	1890
2.8	2.8	28	1400	1960
2.9	2.9	29	1450	2030
3.0	3.0	30	1500	2100
3.1	3.1	31	1550	2170
3.2	3.2	32	1600	2240
3.3	3.3	33	1650	2310
3.4	3.4	34	1700	2380
3.5	3.5	35	1750	2450
3.6	3.6	36	1800	2520



Bluelab Commercial Truncheon® Nutrient Meter product guarantee

Bluelab Corporation Limited guarantees this product for a period of **5 years (60 months)** from the date of sale to the original purchaser. The product will be repaired or replaced, should it be found faulty due to component failure, or faulty workmanship. The faulty product should be returned to the point of purchase.



The guarantee is null and void should any internal parts or fixed external parts be tampered with or altered in any way, or should the unit have been incorrectly operated, or in any way be maltreated. This guarantee does not cover reported faults which are shown to be caused by any or all of the following: contaminated measuring tip (see instruction manual for cleaning instructions), broken glassware or drying of the pH probe glassware, flat or damaged batteries or batteries that have been incorrectly inserted, or damaged battery contacts or connections caused by incorrect battery replacement or ingress of moisture from incorrect positioning of the battery cap and waterproof seal.

NO RESPONSIBILITY will be accepted by Bluelab or any of its agents or resellers should any damage or unfavourable conditions result from the use of this product, should it be faulty or incorrectly operated.

Register your guarantee online at: www.getbluelab.com

Or fill out the form below and post, email or fax to:

Bluelab Corporation Limited

8 Whiore Avenue, Tauriko Industrial Park, Tauranga 3110, New Zealand

Fax: +64 7 578 0847

Email: support@getbluelab.com

Product details

Product name	
Serial number	
Date purchased	

Purchaser details

Purchaser's name	
Address	
City	
Country	
Email (optional)	

Purchased from (Dealers details)

Purchased from	
Address	
City	
Country	
Phone number (optional)	



Bluelab Probe Care Kits

The instrument is only as accurate as the probe is clean!

Probe cleaning is one of the most important parts of owning and operating any Bluelab meter, monitor or controller. If the probe is contaminated (dirty) it affects the accuracy of the reading displayed.

The probe surface is where the instrument takes the reading of the solution. The information is sent back from the probe to the electronic brain of the instrument.

A calculation is then done in the instrument's brain or micro computer and a reading is displayed. If the information sent back from the probe is inaccurate due to probe surface contamination then the reading will be inaccurate. Cleaning the probes is a very easy task and will prolong the life of the probes.



Bluelab Probe Care Kit - pH contents:

- › Cleaning instructions inside box lid
- › 500ml pH4 and pH7 Calibration solutions
- › Decanter vessels
- › Bluelab pH Probe Cleaner
- › Toothbrush (probe cleaning instrument)

Bluelab Probe Care Kit - Conductivity contents:

- › Cleaning instructions inside box lid
- › 500ml 2.77EC conductivity standard solution
- › Decanter vessel
- › Bluelab Conductivity Probe Cleaner
- › Bluelab Chamois (probe cleaning instrument)



If you need assistance or advice - we're here to help you.

Phone: **+64 7 578 0849** Fax: **+64 7 578 0847**

Email: **support@getbluelab.com**



Looking for specifications or technical advice?

Visit us online @ **www.getbluelab.com**



Bluelab Corporation Limited
8 Whiore Avenue, Tauriko Industrial Park
Tauranga 3110, New Zealand



Version 1: TRUNCOMV2_071212_1

© Copyright 2012, all rights reserved, Bluelab Corporation Limited